

End point PCR[†] for MRSA from bacterial colonies

A. Introduction

This protocol uses end point PCR[†] with Minor Groove Binder™ (MGB) TaqMan® probes to test for Methicillin-resistant *Staphylococcus aureus* (MRSA), from bacterial colonies. The two target sequences in this assay are the *mecA* gene for methicillin resistance and the *nuc* gene for a nuclease specific to *S. aureus*.

The Spartan DX™ instrument has a single channel for fluorescence detection. The presence of each gene (*mecA* and *nuc*), and their corresponding negative controls, are tested separately as singleplex reactions.

Approximate time for DNA extraction from bacterial colonies is 20 min. PCR run time is 30 min.

B. Equipment

- Spartan DX instrument
- Microcentrifuge
- Vortex
- Ice bucket or cold block
- Pipettes

C. Materials

- 0.2 ml flat-cap PCR tubes (VWR, Cat. No. 53550-106)
- Filtered pipette tips
- PCR-grade Mineral Oil (Biotools, Cat. No. 20.032)
- QUANTIPROBES™ Reaction Mix (Biotools, Cat. No. 10.601)
- Sterile water (DNase-free)
- TE Buffer (50 mM Tris-HCl, 50 mM NaCl, 5 mM EDTA, pH 8)
- Achromopeptidase (40 U/μl in TE buffer, stored at -20°C) (Sigma-Aldrich, Cat. No. A3547)
- 1.5 ml microcentrifuge tubes
- Primers which recognize *mecA* and *nuc* genes (Sigma-Genosys)(Table 1)
- MGB TaqMan probes for *mecA* and *nuc* genes (Applied Biosystems)(Table 1)

Primer/Probe	Forward (5'-3')	Reverse (5'-3')	Amplicon size (bp)
<i>mecA</i> primers	TCC Agg AAT gCA gAA AgA CCA A	ggC CAA TTC CAC ATT gTT TCg	92
<i>mecA</i> probe	6-FAM-CAT ATT gAA AAT TTA AAA TCA gAA CgT g-MGBNFQ		
<i>nuc</i> primers	gCg ATT gAT ggT gAT ACg gTT	AgC CAA gCC TTg ACg AAC TAA AgC	279
<i>nuc</i> probe	6-FAM CTg AAg CAA gTg CAT TTA-MGBNFQ		

6-FAM = 6-carboxy-fluorescein, MGB = minor groove binder, NFQ = non-fluorescent quencher

Table 1. Primer/probe sequences and amplicon sizes.

D. Preparation

1. With a sterile transfer device, pick 4 bacterial colonies from a culture plate
2. Resuspend colonies in 200 μl of TE buffer, with 5 μl of 40 U/μl achromopeptidase
3. Incubate at 30°C for 10 min
4. Boil samples for 10 min to inactivate achromopeptidase
5. Turn on Spartan DX instrument and let it warm up for a minimum of 10 min
6. Set up cycling program as per Table 2

Step	Temperature	Time	Cycles
Initial denaturation	95°C	44 s	1
Denaturation	95°C	16 s	40
Annealing/extension	57°C	26 s	40

Table 2. Cycling parameters.

E. Protocol

1. Prepare two separate *mecA* and *nuc* master mixes, as per Table 3
2. Since the Spartan DX instrument holds 4 tubes, we recommend setting up reactions as follows:
 - Tube 1: 18 µl of *mecA* master mix
 - Tube 2: 18 µl of *nuc* master mix
 - Tube 3: 18 µl of *mecA* master mix
 - Tube 4: 18 µl of *nuc* master mix
3. In a separate lab area add the following to each tube:
 - Tube 1: 2 µl of extracted DNA (sample in question)
 - Tube 2: 2 µl of extracted DNA (sample in question)
 - Tube 3: 2 µl of sterile water (*mecA* negative control)
 - Tube 4: 2 µl of sterile water (*nuc* negative control)
4. Mix and spin down reactions
5. Overlay reaction mixture with 15 µl of mineral oil
6. Spin down reactions again
7. Insert tubes into Spartan DX instrument and start your run
8. End point PCR is determined to be positive if the last cycle reading has a fluorescence value greater than 5
9. Table 4 lists possible genotypes.

Reagent	<i>mecA</i> Master Mix		<i>nuc</i> Master Mix	
	Reaction Formulation	Volume	Reaction Formulation	Volume
QUANTIPROBES Reaction Mix (2X)	10 µl x (____+0.5*) Sample #		10 µl x (____+0.5*) Sample #	
Forward primer (10 µM)	2 µl x (____+0.5*) Sample #		2 µl x (____+0.5*) Sample #	
Reverse primer (10 µM)	2 µl x (____+0.5*) Sample #		2 µl x (____+0.5*) Sample #	
Probe (0.5 µM)	2 µl x (____+0.5*) Sample #		2 µl x (____+0.5*) Sample #	
Sterile water	2 µl x (____+0.5*) Sample #		2 µl x (____+0.5*) Sample #	
Total volume of master mix	18 µl/reaction	____ µl	18 µl/reaction	____ µl

* Recommended volume correction factor for pipetting error.

Table 3. Primer/probe mixes for *mecA* and *nuc*.

Genotype	<i>mecA</i>	<i>nuc</i>
MRSA (Methicillin-resistant <i>Staphylococcus aureus</i>)	+	+
MSSA (Methicillin-sensitive <i>Staphylococcus aureus</i>)	-	+
MR-CNS (Methicillin-resistant coagulase-negative <i>Staphylococci</i>)	+	-
MS-CNS (Methicillin-sensitive coagulase-negative <i>Staphylococci</i>)	-	-

Table 4. Possible genotypes.

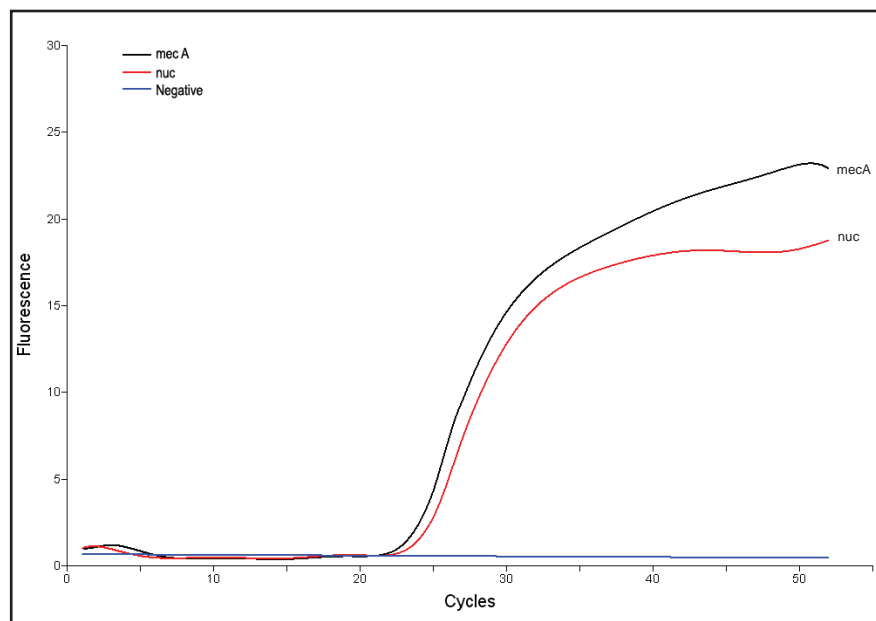


Figure 1. Real-time graph of MRSA results.

† - An end point assay is described as an assay that uses data from images collected at the first and last cycles of a PCR run to determine the success or failure of the reaction. End point analysis mode is selected in the options menu of the SpartanDX™.

Disclaimer

PCR and real-time PCR processes are covered by patents issued and applicable in certain countries. This product is not licensed under these patents. Spartan does not encourage or support the unauthorized or unlicensed use of PCR or real-time PCR processes. Use of this instrument is recommended for persons that either have licenses to perform PCR and real-time PCR, or are not required to obtain licenses. Users interested in obtaining a license for these patents should contact the respective patent and license owners.

Trademarks

Spartan DX™ is a registered trademark of Spartan Bioscience Inc. All other trademarks are the sole property of their respective owners.